

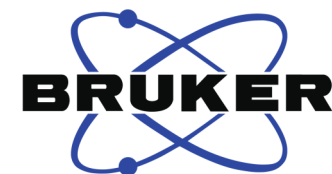


m/z 389

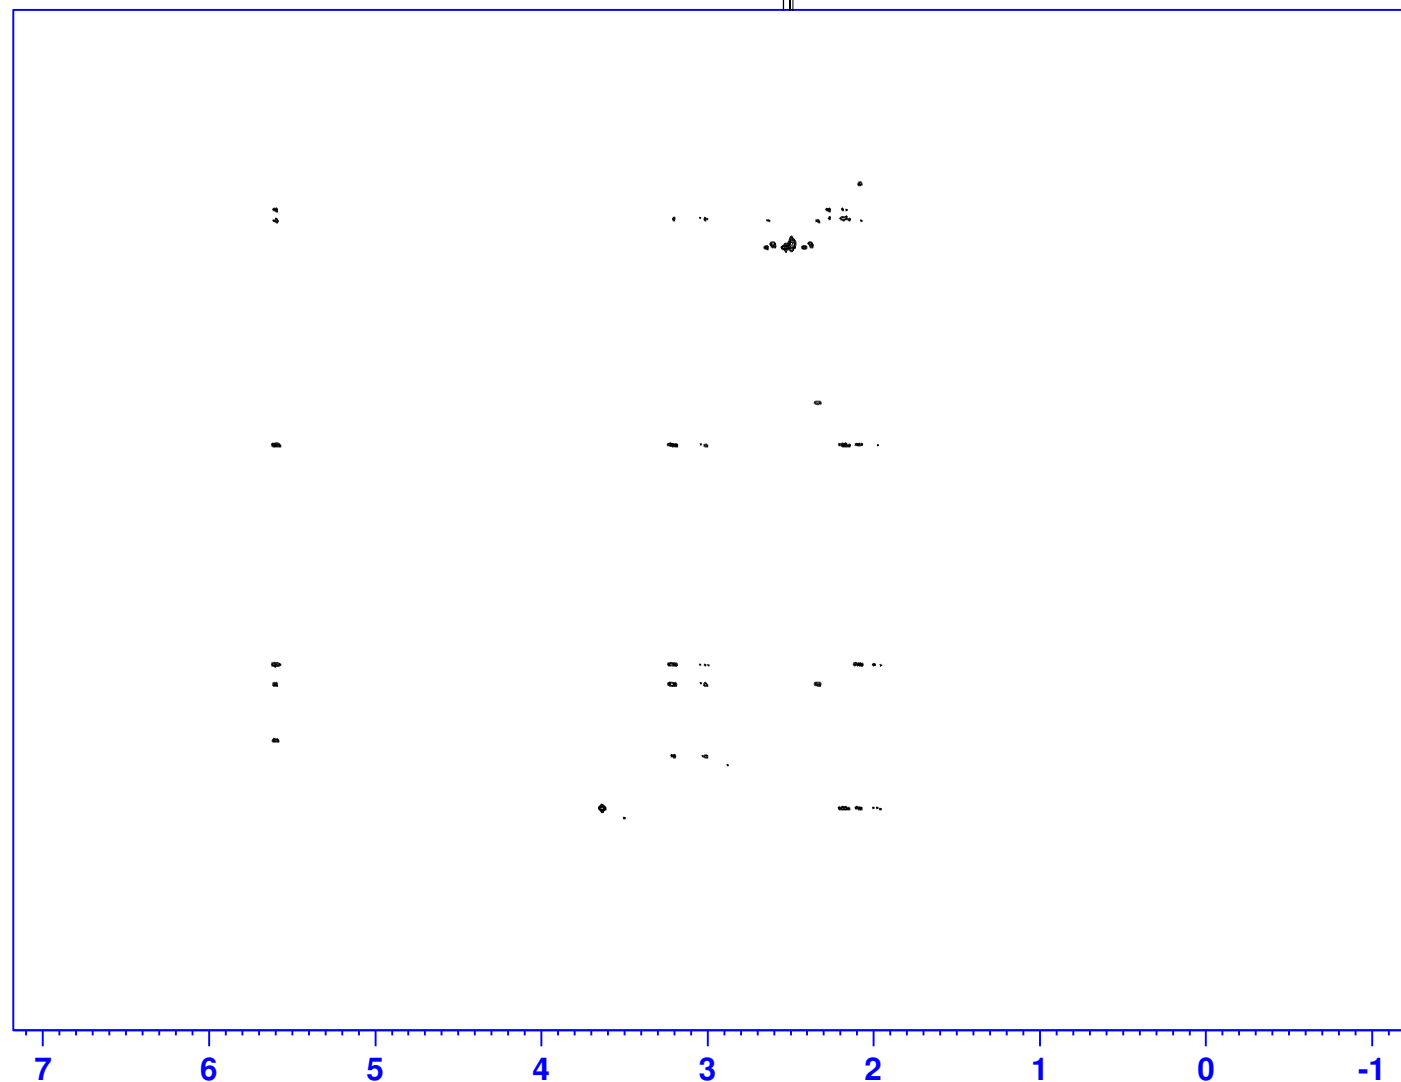

Current Data Parameters
NAME WKU285
EXPNO 58
PROCNO 1

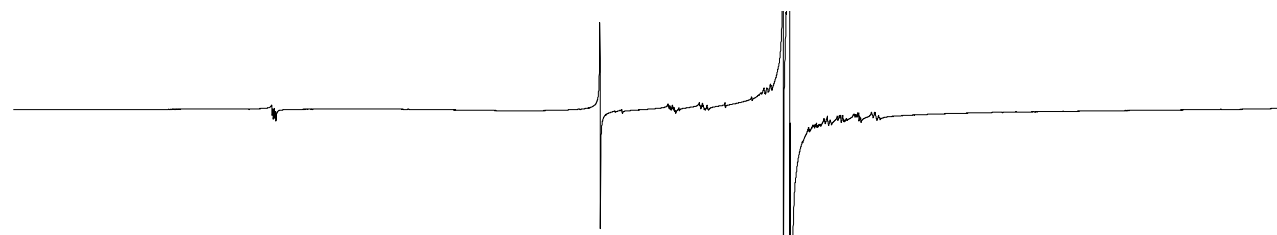

ppm

0 F2 - Acquisition Parameters
Date_ 20191109
Time 20.10 h
INSTRUM spect
PROBHD Z126545_0009 (
PULPROG hmbcgp1pndgf
TD 4096
SOLVENT DMSO
NS 96
DS 16
SWH 5050.505 Hz
FIDRES 2.466067 Hz
AQ 0.4055040 sec
RG 194.73
DW 99.000 usec
DE 28.00 usec
40 TE 298.0 K
CNST2 145.0000000
CNST13 8.0000000
D0 0.00000300 sec
D1 1.37848496 sec
60 D2 0.00344828 sec
D6 0.06250000 sec
D16 0.00020000 sec
IN0 0.00001380 sec
SPARSELI 0
80 TDav 1
SFO1 600.1517840 MHz
NUC1 1H
P1 12.00 usec
P2 24.00 usec
100 PLW1 24.71599960 W
SFO2 150.9236829 MHz
NUC2 13C
P3 10.00 usec
PLW2 58.00000000 W
GPNAM[1] SMSQ10.100
120 GPZ1 50.00 %
GPNAM[2] SMSQ10.100
GPZ2 30.00 %
GPNAM[3] SMSQ10.100
140 GPZ3 40.10 %
P16 1000.00 usec

F1 - Acquisition parameters
TD 128
SFO1 150.9237 MHz
160 FIDRES 566.123169 Hz
SW 240.068 ppm
FnMODE QF

F2 - Processing parameters
SI 2048
SF 600.1500000 MHz
WDW SINE
SSB 0
LB 0 Hz
200 GB 0
PC 1.40

F1 - Processing parameters
SI 1024
MC2 QF
220 SF 150.9078375 MHz
WDW SINE
SSB 0
LB 0 Hz
GB 0