


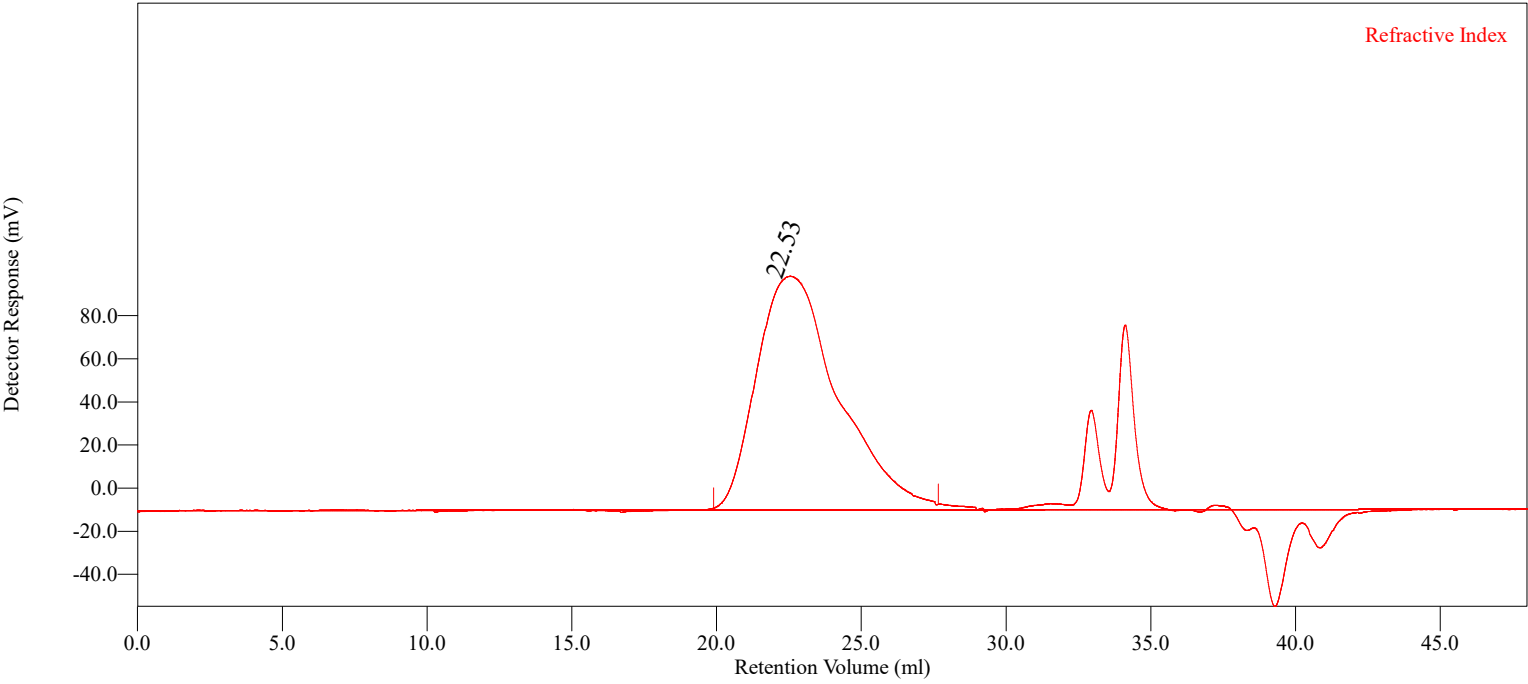

Warning: No flow rate marker was found.

Conventional Calibration - Homopolymers : Results

Peak RV - (ml)	22.531
Mn - (Daltons)	28,355
Mw - (Daltons)	53,531
Mz - (Daltons)	85,612
Mp - (Daltons)	51,787
Mw / Mn	1.888
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	9,185
Mw 10.0% High	147,101
Wt Fr (Peak)	1.000
RI Area - (mvml)	353.95
UV Area - (mvml)	0.00

Annotation	
Method File	convcal_PS1-0000.vcm
Limits File	
Date Acquired	Apr 17, 2025 - 02:33:02
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	PSS SDV 100,1000,100000
System	Triple Detection
Flow Rate - (ml/min)	0.800
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00267
Detector Temp. - (deg C)	35.0
Column Temp. - (deg C)	35.0
OmniSEC Build Number	461

