


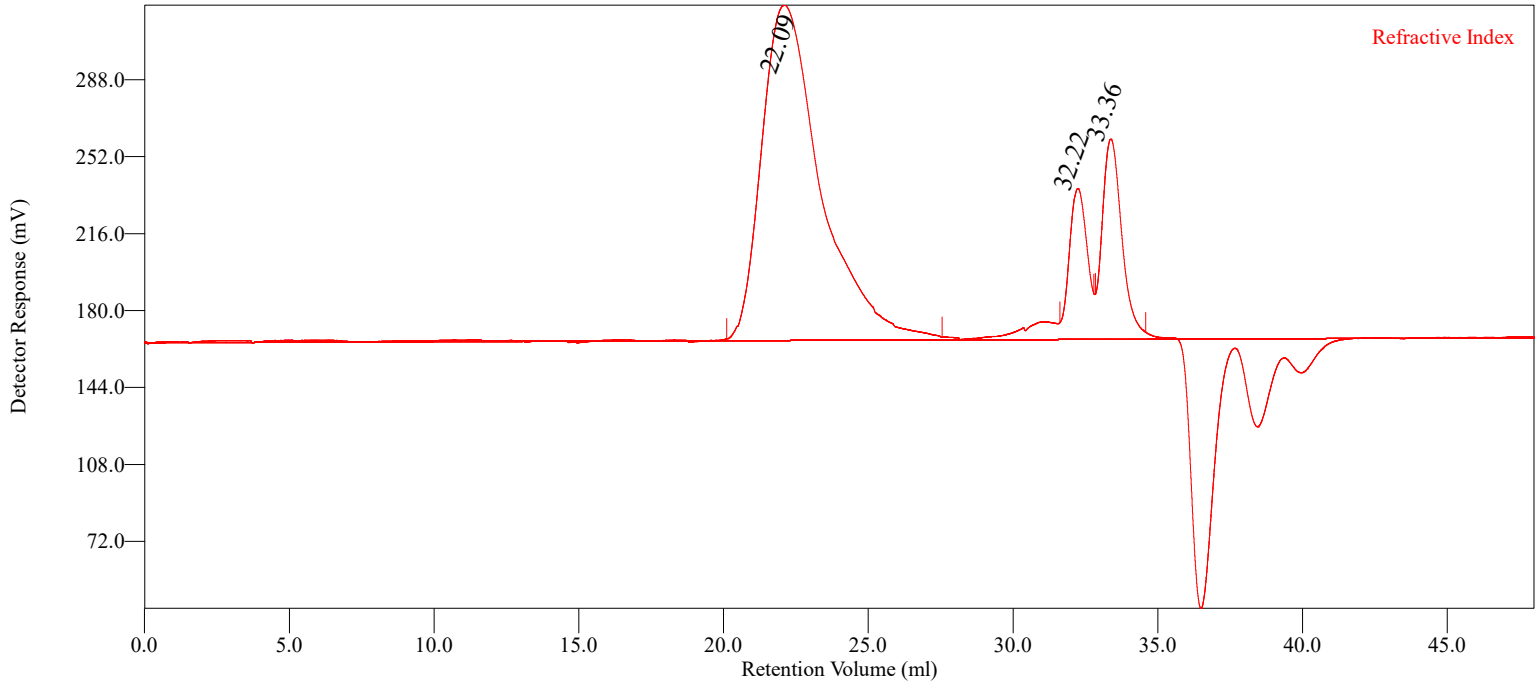

Warning: No flow rate marker was found.

Conventional Calibration - Homopolymers : Results

Peak RV - (ml)	22.088	32.224	33.363
Mn - (Daltons)	38,922	604	358
Mw - (Daltons)	62,924	611	366
Mz - (Daltons)	85,502	619	373
Mp - (Daltons)	68,506	614	378
Mw / Mn	1.617	1.012	1.021
Percent Above Mw: 0	100.000	100.000	100.000
Percent Below Mw: 0	0.000	0.000	0.000
Mw 10.0% Low	13,367	505	270
Mw 10.0% High	141,858	731	448
Wt Fr (Peak)	0.749	0.102	0.149
RI Area - (mvml)	371.71	50.60	73.89
UV Area - (mvml)	0.00	0.00	0.00

Annotation	
Method File	convcal_PS1-0000.vcm
Limits File	
Date Acquired	May 15, 2025 - 19:26:15
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	PSS SDV 100,1000,100000
System	Triple Detection
Flow Rate - (ml/min)	0.800
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00267
Detector Temp. - (deg C)	35.0
Column Temp. - (deg C)	35.0
OmniSEC Build Number	461

