




Conventional Calibration - Homopolymers : Results

Peak RV - (ml)	21.227	34.123
Mn - (Daltons)	43,994	0
Mw - (Daltons)	125,848	0
Mz - (Daltons)	266,944	0
Mp - (Daltons)	116,860	0
Mw / Mn	2.861	0.000
Percent Above Mw: 0	100.000	0.000
Percent Below Mw: 0	0.000	0.000
Mw 10.0% Low	12,114	0
Mw 10.0% High	437,824	0
Wt Fr (Peak)	1.000	0.000
RI Area - (mvml)	242.84	52.49
UV Area - (mvml)	0.00	0.00

Annotation	
Method File	convcal PS1-0000.vcm
Limits File	
Date Acquired	Apr 17, 2025 - 01:31:50
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	PSS SDV 100,1000,100000
System	Triple Detection
Flow Rate - (ml/min)	0.800
lnj Volume - (ul)	100.0
Volume Increment - (ml)	0.00267
Detector Temp. - (deg C)	35.0
Column Temp. - (deg C)	35.0
OmniSEC Build Number	461

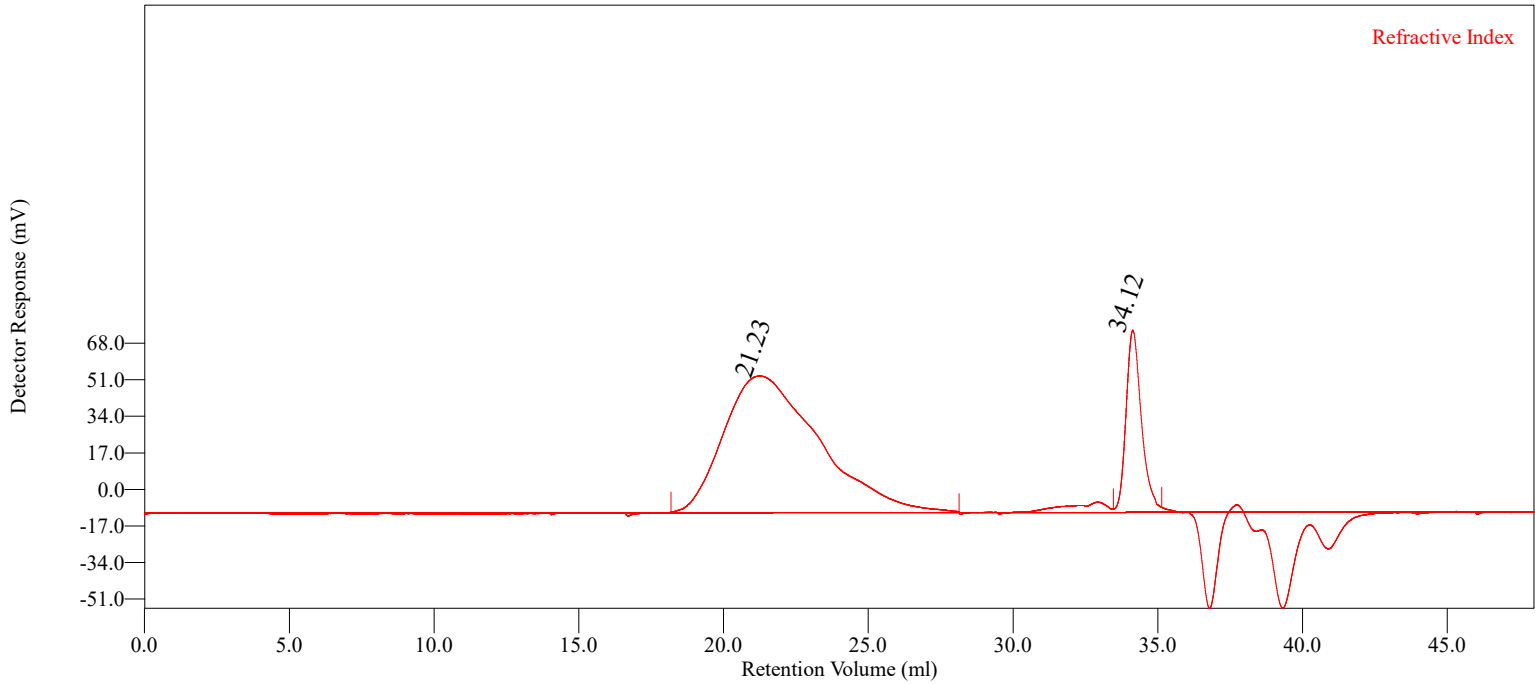